

REFERENCE

NBS
PUBLICATIONS




NBS TECHNICAL NOTE 1083

U.S. DEPARTMENT OF COMMERCE / National Bureau of Standards

A Radio-Frequency Power Delivery System: Procedures for Error Analysis and Self-Calibration

Motohisa Kanda
R. David Orr

QC
100
.U5753
No. 1083
1985



The National Bureau of Standards¹ was established by an act of Congress on March 3, 1901. The Bureau's overall goal is to strengthen and advance the nation's science and technology and facilitate their effective application for public benefit. To this end, the Bureau conducts research and provides: (1) a basis for the nation's physical measurement system, (2) scientific and technological services for industry and government, (3) a technical basis for equity in trade, and (4) technical services to promote public safety. The Bureau's technical work is performed by the National Measurement Laboratory, the National Engineering Laboratory, the Institute for Computer Sciences and Technology, and the Center for Materials Science.

The National Measurement Laboratory

Provides the national system of physical and chemical measurement; coordinates the system with measurement systems of other nations and furnishes essential services leading to accurate and uniform physical and chemical measurement throughout the Nation's scientific community, industry, and commerce; provides advisory and research services to other Government agencies; conducts physical and chemical research; develops, produces, and distributes Standard Reference Materials; and provides calibration services. The Laboratory consists of the following centers:

- Basic Standards²
- Radiation Research
- Chemical Physics
- Analytical Chemistry

The National Engineering Laboratory

Provides technology and technical services to the public and private sectors to address national needs and to solve national problems; conducts research in engineering and applied science in support of these efforts; builds and maintains competence in the necessary disciplines required to carry out this research and technical service; develops engineering data and measurement capabilities; provides engineering measurement traceability services; develops test methods and proposes engineering standards and code changes; develops and proposes new engineering practices; and develops and improves mechanisms to transfer results of its research to the ultimate user. The Laboratory consists of the following centers:

- Applied Mathematics
- Electronics and Electrical Engineering²
- Manufacturing Engineering
- Building Technology
- Fire Research
- Chemical Engineering²

The Institute for Computer Sciences and Technology

Conducts research and provides scientific and technical services to aid Federal agencies in the selection, acquisition, application, and use of computer technology to improve effectiveness and economy in Government operations in accordance with Public Law 89-306 (40 U.S.C. 759), relevant Executive Orders, and other directives; carries out this mission by managing the Federal Information Processing Standards Program, developing Federal ADP standards guidelines, and managing Federal participation in ADP voluntary standardization activities; provides scientific and technological advisory services and assistance to Federal agencies; and provides the technical foundation for computer-related policies of the Federal Government. The Institute consists of the following centers:

- Programming Science and Technology
- Computer Systems Engineering

The Center for Materials Science

Conducts research and provides measurements, data, standards, reference materials, quantitative understanding and other technical information fundamental to the processing, structure, properties and performance of materials; addresses the scientific basis for new advanced materials technologies; plans research around cross-country scientific themes such as nondestructive evaluation and phase diagram development; oversees Bureau-wide technical programs in nuclear reactor radiation research and nondestructive evaluation; and broadly disseminates generic technical information resulting from its programs. The Center consists of the following Divisions:

- Inorganic Materials
- Fracture and Deformation³
- Polymers
- Metallurgy
- Reactor Radiation

¹Headquarters and Laboratories at Gaithersburg, MD, unless otherwise noted; mailing address Gaithersburg, MD 20899.

²Some divisions within the center are located at Boulder, CO 80303.

³Located at Boulder, CO, with some elements at Gaithersburg, MD.

A Radio-Frequency Power Delivery System: Procedures for Error Analysis and Self-Calibration

Motohisa Kanda
R. David Orr

Electromagnetic Fields Division
Center for Electronics and Electrical Engineering
National Engineering Laboratory
National Bureau of Standards
Boulder, Colorado 80303



U.S. DEPARTMENT OF COMMERCE, Malcolm Baldrige, Secretary

NATIONAL BUREAU OF STANDARDS, Ernest Ambler, Director

Issued August 1985

National Bureau of Standards Technical Note 1083
Natl. Bur. Stand. (U.S.), Tech Note 1083, 24 pages (Aug. 1985)
CODEN:NBTNAE

U.S. GOVERNMENT PRINTING OFFICE
WASHINGTON: 1985

For sale by the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20402

CONTENTS

	Page
1. Introduction.....	1
2. System S-Parameters.....	1
3. Expressions for Net Delivered Power.....	3
4. A Self-Calibrating System.....	7
5. Summary of Self-Calibration Procedure.....	9
6. Estimated Uncertainty in Computed Net Power.....	11
7. Conclusion.....	15
8. Acknowledgment.....	15
9. References.....	16

A RADIO-FREQUENCY POWER DELIVERY SYSTEM:
PROCEDURES FOR ERROR ANALYSIS AND SELF-CALIBRATION

Motohisa Kanda and R. David Orr

Electromagnetic Fields Division
National Bureau of Standards
Boulder, Colorado 80303

An expression is developed for net power delivered to a load in terms of the indicated forward and reflected power and the system S-parameters and reflection coefficients. The dual directional coupler is treated as nonideal with power reflections assumed between all ports. The system itself is used to evaluate the major S-parameter terms in net power computation, and uncertainty in the computed power is derived from origins in the power meter readings and incompletely known S-parameters.

Key words: errors; error analysis; radio-frequency power; scattering coefficients; S-parameters.

1. Introduction

Standard-gain horn antennas are employed to establish known electromagnetic (EM) fields in the National Bureau of Standards anechoic chamber. Part of the uncertainty in our knowledge of these fields arises from the uncertainty in the net power delivered to the horn. In turn, this uncertainty reflects our lack of knowledge of the amplitudes and phases of the various reflection and transmission coefficients in the power delivery system, as well as the uncertainty in measurements of the power incident upon and reflected from the horn. To determine how the net power to an antenna depends on system components, we now derive an expression for net power in terms of power meter readings and the system S (scattering)-parameters.

2. System S-Parameters

We derive our net power expression from a set of simultaneous S-parameter equations which describe voltage waves at an n-port microwave junction. In figure 1, the voltage wave a_j is incident on port j when all other ports have matched terminations. The voltage wave b_i emerging into the termination on port i is obtained from the incident wave a_j at port j by the relation defining the S-parameter S_{ij} [1]:

$$b_i = S_{ij} a_j. \quad (1)$$

The symbols b_i and a_j are complex and represent the magnitude and phase of the waves at ports i and j ; S_{ij} , therefore, is also complex. (For convenience in writing the power equations that appear later, we let a and b represent voltage, i.e. E field, waves normalized to $\sqrt{Z_0}$, the square root of the characteristic impedance of the system.) When $i = j$, the S-parameter is a reflection coefficient; when $i \neq j$, the S-parameter is a transmission coefficient.

If all the ports are terminated in unmatched loads, there will be an incident a_j at every j^{th} port contributing to the voltage wave b_i emerging from the i^{th} port:

$$b_i = S_{i1}a_1 + S_{i2}a_2 + \dots S_{ij}a_j + \dots S_{in}a_n. \quad (2)$$

Because a similar equation can be written for the voltage wave emerging from every i^{th} port, we have a set of n simultaneous equations in which all emerging waves are related to all incident waves through the S-parameters S_{ij} of the junction.

In our system for establishing standard radio-frequency fields, we compute net power delivered to the transmitting antenna from measurements of incident and reflected power obtained with a dual directional coupler. Our power delivery and measurement system can, therefore, be represented as shown in figure 2 where the port terminations and numbering are:

1. Power meter to monitor forward power
2. Power meter to monitor power reflected from antenna
3. Rf generator
4. Antenna (load).

We now confine our attention to that part of the system in figure 2 within the dashed rectangle and, except for their action as "reflectors" (imperfect matches), we exclude the four terminations. This four-port system, including such components as dual directional coupler, switches, and cables is described by four simultaneous S-parameter equations:

$$\begin{aligned}
b_1 &= S_{11}a_1 + S_{12}a_2 + S_{13}a_3 + S_{14}a_4 \\
b_2 &= S_{21}a_1 + S_{22}a_2 + S_{23}a_3 + S_{24}a_4 \\
b_3 &= S_{31}a_1 + S_{32}a_2 + S_{33}a_3 + S_{34}a_4 \\
b_4 &= S_{41}a_1 + S_{42}a_2 + S_{43}a_3 + S_{44}a_4
\end{aligned} \tag{3}$$

Again, each b_i represents the magnitude and phase of a voltage wave emerging from the i^{th} port, and a_j the magnitude and phase of a voltage wave incident at the j^{th} port. Because the system (everything within the dashed-line rectangle in figure 2) described by these equations is reciprocal [1], we use the reciprocity condition

$$S_{ij} = S_{ji} \tag{4}$$

to simplify the simultaneous equations. (The reciprocity condition is $S_{ij}Z_j = S_{ji}Z_i$; but we assume $Z_j = Z_i$.) Solving these equations for b_i/b_j is further simplified by relating each b_i to a_i through the voltage reflection coefficient Γ_i of the termination on the i^{th} port:

$$a_1 = b_1\Gamma_1; a_2 = b_2\Gamma_2; a_4 = b_4\Gamma_4. \tag{5}$$

3. Expressions for Net Delivered Power

An expression for net power absorbed by the load can be obtained from inspection of figure 2 if we assume an ideal dual directional coupler. By that, we mean a coupler in which there is complete isolation between ports 1 and 4, 2 and 3, and 1 and 2; i.e., $S_{14} = S_{23} = S_{12} = 0$. Thus, the power emerging from port 1 is derived only from the generator power entering at port 3; and the power emerging from port 2 is derived only from power entering port 4 in the voltage wave reflected from the load on port 4. The power absorbed by a load on port 4 is the difference between incident and reflected power at the load: $P_{\text{net}} = P_{\text{inc}} - P_{\text{refl}}$. Then, where b_4 and a_4 are the emerging and incident waves at port 4 and Γ_4 is the voltage reflection coefficient of the port 4 load,

$$P_{\text{net}} = |b_4|^2 - |a_4|^2 = |b_4|^2 - |b_4\Gamma_4|^2 = |b_4|^2 (1 - |\Gamma_4|^2). \tag{6}$$

Keeping in mind that the power transmission coefficient $|S_{ij}|^2$ represents an attenuation and that P_i is the reading of a power meter whose sensor has a reflection coefficient Γ_i , we inspect figure 2 and write an expression for the power incident on the port 4 load in terms of P_1 . The power $|b_1|^2$ emerging from port 1 is P_1 divided by $1 - |\Gamma_1|^2$ (i.e., $P_1 = |b_1|^2 \times (1 - |\Gamma_1|^2)$); $|b_1|^2$ divided by $|S_{13}|^2$ is the power entering the coupler at port 3; and this power multiplied by $|S_{34}|^2$ is the power emerging from port 4. Using similar reasoning to relate $|b_2|^2$ to the power reflected from the load, we have

$$P_{\text{inc}} = \frac{P_1 |S_{34}|^2}{|S_{13}|^2 (1 - |\Gamma_1|^2)} \quad ; \quad P_{\text{refl}} = \frac{P_2}{|S_{24}|^2 (1 - |\Gamma_2|^2)}. \quad (7)$$

The power absorbed by the load antenna in the idealized system is now

$$\begin{aligned} P_{\text{net}} &= \frac{P_1 |S_{34}|^2}{|S_{13}|^2 (1 - |\Gamma_1|^2)} - \frac{P_2}{|S_{24}|^2 (1 - |\Gamma_2|^2)} \\ &= \left| \frac{S_{34}}{S_{13}} \right|^2 \frac{P_1}{1 - |\Gamma_1|^2} - \frac{1}{|S_{24}|^2} \frac{P_2}{1 - |\Gamma_2|^2}. \end{aligned} \quad (8)$$

This equation tells us which parameters of this ideal system we must know in order to compute P_{net} from power measurements P_1 and P_2 .

We now derive an expression for P_{net} for a real (i.e., nonideal) four-port system in which none of the $S_{ij} = 0$.

$$P_{\text{net}} = P_{\text{inc}} - P_{\text{refl}} = |b_4|^2 - |a_4|^2; \quad a_4 = b_4 \Gamma_4 \quad (9)$$

where Γ_4 is the reflection coefficient of the load. Because our power measurements are made at ports 1 and 2, we want to express b_4 in terms of b_1 , and a_4 in terms of b_2 . We do this by solving eq (3) for b_4/b_1 and b_4/b_2 :

$$\frac{b_4}{b_1} = g(S, \Gamma); \quad \frac{b_4}{b_2} = \frac{a_4}{b_2 \Gamma_4} = h(S, \Gamma) \quad (10)$$

where $g(S, \Gamma)$ and $h(S, \Gamma)$ are functions of the system S-parameters and the reflection coefficients of terminations on ports 1, 2, and 4. Now

$$P_{\text{net}} = |b_1|^2 |g|^2 - |b_2|^2 |\Gamma_4|^2 |h|^2. \quad (11)$$

The quantities b_1 and b_2 can be expressed in terms of the power meter readings at ports 1 and 2 by using the final form of eq (6):

$$P_1 = |b_1|^2(1 - |\Gamma_1|^2); P_2 = |b_2|^2(1 - |\Gamma_2|^2) \quad (12)$$

and so

$$P_{\text{net}} = \frac{P_1}{1 - |\Gamma_1|^2} |g|^2 - \frac{P_2 |\Gamma_4|^2}{1 - |\Gamma_2|^2} |h|^2. \quad (13)$$

To obtain g and h , we modify eq (3) by using the reciprocity relation (eq (4)) and eq (5) ($a_i = b_i \Gamma_i$). The voltage wave b_3 is not involved in our computations for P_{net} and so we use only the first two and the fourth of eq (3). These are now:

$$\begin{aligned} b_1 &= S_{11}\Gamma_1 b_1 + S_{12}\Gamma_2 b_2 + S_{13}a_3 + S_{14}\Gamma_4 b_4 \\ b_2 &= S_{12}\Gamma_1 b_1 + S_{22}\Gamma_2 b_2 + S_{23}a_3 + S_{24}\Gamma_4 b_4 \\ b_4 &= S_{14}\Gamma_1 b_1 + S_{24}\Gamma_2 b_2 + S_{34}a_3 + S_{44}\Gamma_4 b_4. \end{aligned} \quad (14)$$

A convenient form for these equations can be obtained by grouping the two common b_i terms within each equation, then solving the first for a_3 and substituting this for a_3 in the second and third equations (this treatment is based on [2]). We then have

$$\begin{aligned} -Bb_1 &= -Ab_2 + Cb_4 \\ -Eb_1 &= Fb_2 - Db_4 \end{aligned} \quad (15)$$

where

$$\begin{aligned} A &= S_{13} (1 - S_{22}\Gamma_2) + S_{12}S_{23}\Gamma_2 \\ B &= S_{23} (1 - S_{11}\Gamma_1) + S_{12}S_{13}\Gamma_1 \\ C &= (S_{13}S_{24} - S_{14}S_{23})\Gamma_4 \\ D &= S_{13} (1 - S_{44}\Gamma_4) + S_{14}S_{34}\Gamma_4 \\ E &= S_{34} (1 - S_{11}\Gamma_1) + S_{13}S_{14}\Gamma_1 \\ F &= (S_{13}S_{24} - S_{12}S_{34})\Gamma_2. \end{aligned} \quad (16)$$

Equation (15) can now be solved for the ratios $g(S, \Gamma) = b_4/b_1$ and $h(S, \Gamma) = b_4/b_2$, giving the following expressions for g and h in eq (13) for P_{net} :

$$g(S, \Gamma) = \frac{S_{34}}{S_{13}} \times \frac{1 - S_{11}\Gamma_1}{1 - S_{44}\Gamma_4} \times \frac{1 + \frac{S_{13}S_{14}\Gamma_1}{S_{34}(1 - S_{11}\Gamma_1)}}{1 + \frac{S_{14}S_{34}\Gamma_4}{S_{13}(1 - S_{44}\Gamma_4)}} \quad (17)$$

$$\begin{aligned} & \times \frac{1 + \frac{[S_{23}(1 - S_{11}\Gamma_1) + S_{12}S_{13}\Gamma_1](S_{13}S_{24} - S_{12}S_{34})\Gamma_2}{[S_{13}(1 - S_{22}\Gamma_2) + S_{12}S_{23}\Gamma_2][S_{34}(1 - S_{11}\Gamma_1) + S_{13}S_{14}\Gamma_1]}}{1 - \frac{(S_{13}S_{24} - S_{14}S_{23})(S_{13}S_{24} - S_{12}S_{34})\Gamma_2\Gamma_4}{[S_{13}(1 - S_{22}\Gamma_2) + S_{12}S_{23}\Gamma_2][S_{13}(1 - S_{44}\Gamma_4) + S_{14}S_{34}\Gamma_4]}} \\ h(S, \Gamma) &= \frac{1}{S_{24}} \times \frac{1 - S_{22}\Gamma_2}{\Gamma_4} \times \frac{1 + \frac{S_{12}S_{23}\Gamma_2}{S_{13}(1 - S_{22}\Gamma_2)}}{1 - \frac{S_{14}S_{23}}{S_{13}S_{24}}} \end{aligned} \quad (18)$$

$$\begin{aligned} & \times \frac{1 + \frac{[S_{23}(1 - S_{11}\Gamma_1) + S_{12}S_{13}\Gamma_1](S_{13}S_{24} - S_{12}S_{34})\Gamma_2}{[S_{13}(1 - S_{22}\Gamma_2) + S_{12}S_{23}\Gamma_2][S_{34}(1 - S_{11}\Gamma_1) + S_{13}S_{14}\Gamma_1]}}{1 + \frac{[S_{23}(1 - S_{11}\Gamma_1) + S_{12}S_{13}\Gamma_1][S_{13}(1 - S_{44}\Gamma_4) + S_{14}S_{34}\Gamma_4]}{[S_{34}(1 - S_{11}\Gamma_1) + S_{13}S_{14}\Gamma_1](S_{13}S_{24} - S_{14}S_{23})\Gamma_4}} \end{aligned}$$

We see that the initial factors in g and h are S_{34}/S_{13} and $1/S_{24}$, respectively. These factors are present in eq (8) for the P_{net} in an idealized system. Thus, the rest of g and h corrects eq (8) for a system which is not ideal. (Note that the second term in h contains $1/\Gamma_4$ which removes the considerable dependence on Γ_4 that P_{net} appears to have in eq (13)). Section 6 further discusses the role of g and h in determining the uncertainty in P_{net} due to approximating eq (13) with eq (8).

If the S -parameters, reflection coefficients, and their uncertainties are known for our four-port system, we can use eq (13) to compute P_{net} and its uncertainty from the power measurements P_1 and P_2 and their uncertainties. The amplitudes of some of the S_{ij} (see page 11) are so much less than unity that P_{net} should be a weak function of their phases. To confirm this we computed g and h using these S_{ij} and Γ_i magnitudes. We allowed for a complete lack of phase information for these parameters by replacing each plus and minus sign in eqs (17) and (18) with a \pm sign. The uncertainty in P_{net} introduced by this phase

ambiguity is only ± 1.2 percent when $|\Gamma_4| = 0.05$. For this reason, an order-of-magnitude knowledge of some of the S_{ij} amplitudes is sufficient for evaluating g and h . Uncertainty components in P_{net} are discussed further in section 6.

4. A Self-Calibrating System

The functions $g(S, \Gamma)$ and $h(S, \Gamma)$ were written in the forms given in eqs (17) and (18) to show which S -parameters have the most direct influence on P_{net} . These parameters (S_{13} , S_{24} , and S_{34}) predominate in g and h in the forms S_{34}/S_{13} and $1/S_{24}$, and in P_{net} as squares of magnitudes $|S_{34}/S_{13}|^2$ and $|1/S_{24}|^2$ which do not involve the parameter phases. One of our intentions in developing an automated system for establishing standard electromagnetic fields is to make the system largely self-calibrating in the sense that the system itself is used to evaluate $|S_{34}/S_{13}|^2$ and $|1/S_{24}|^2$. This section presents the procedures for such a "self analysis".

In figure 3a, we have replaced the load on port 4 with a short ($\Gamma_4 = -1$). Using eq (12), the ratio of power measurements P_2 and P_1 is

$$\frac{P_2}{P_1} = \left| \frac{b_2}{b_1} \right|^2 \frac{1 - |\Gamma_2|^2}{1 - |\Gamma_1|^2} \quad (19)$$

We solve eq (15) for b_2/b_1 and obtain

$$\begin{aligned} \left| \frac{b_2}{b_1} \right|^2 &= |\Gamma_4|^2 \times \left| \frac{S_{24}S_{34}}{S_{13}} \right|^2 \times \left| \frac{1 - S_{11}\Gamma_1}{(1 - S_{44}\Gamma_4)(1 - S_{22}\Gamma_2)} \right|^2 \\ &\times \left| \frac{1 - \frac{S_{14}S_{23}}{S_{13}S_{24}}}{1 + \frac{S_{12}S_{23}\Gamma_2}{S_{13}(1 - S_{22}\Gamma_2)}} \right|^2 \times \left| \frac{1 + \frac{S_{13}S_{14}\Gamma_1}{S_{34}(1 - S_{11}\Gamma_1)}}{1 + \frac{S_{14}S_{34}\Gamma_4}{S_{13}(1 - S_{44}\Gamma_4)}} \right|^2 \\ &\times \left| \frac{1 - \frac{[S_{23}(1 - S_{11}\Gamma_1) + S_{12}S_{13}\Gamma_1][S_{13}(1 - S_{44}\Gamma_4) + S_{14}S_{34}\Gamma_4]}{[S_{34}(1 - S_{11}\Gamma_1) + S_{13}S_{14}\Gamma_1](S_{14}S_{23} - S_{13}S_{24})\Gamma_4}}}{1 - \frac{(S_{14}S_{23} - S_{13}S_{24})(S_{12}S_{34} - S_{13}S_{24})\Gamma_2\Gamma_4}{[S_{13}(1 - S_{44}\Gamma_4) + S_{14}S_{34}\Gamma_4][S_{13}(1 - S_{22}\Gamma_2) + S_{12}S_{23}\Gamma_2]}} \right|^2 \end{aligned} \quad (20)$$

in which $|\Gamma_4| = 1$. Writing this equation in this form (with $|\Gamma_4| = 1$) shows that $|b_2/b_1|^2$ depends primarily on the first term containing the squares of magnitudes of S_{24} , S_{34} , and S_{13} . For a typical dual directional coupler, the S_{ij} magnitudes are such that the numerators and denominators of the last four terms can be written as unity with a small number added or subtracted. Because we do not know the phases of the S-parameters, the value of each S_{ij} may be anywhere from $+|S_{ij}|$ to $-|S_{ij}|$ (similarly for the Γ s). Therefore, the last four terms in eq (20) can each be put in the form $|1 \pm (\text{a small number})|^2$ and then the expression for $|b_2/b_1|^2$ reduced to

$$\left| \frac{b_2}{b_1} \right|^2 = \left| \frac{S_{24}S_{34}}{S_{13}} \right|^2 (1 \pm \Delta) \quad (21)$$

where Δ is the uncertainty in $|b_2/b_1|^2$. The order of Δ can be obtained by substituting nominal values for the S_{ij} and Γ s into eq (20). From eqs (19,21) we now have

$$\left| \frac{S_{24}S_{34}}{S_{13}} \right|^2 = \frac{P_2}{P_1(1 \pm \Delta)} \frac{1 - |\Gamma_1|^2}{1 - |\Gamma_2|^2} \quad (22)$$

where Δ and the uncertainty in P_2/P_1 make up the total uncertainty in $|S_{24}S_{34}/S_{13}|^2$. The reflection coefficients Γ_1 and Γ_2 are given in the manufacturer's specifications for the power meter sensors on ports 1 and 2. (Because our uncertainty estimates are derived from phase ambiguities, the Γ_1 and Γ_2 magnitudes do not contribute to the total uncertainty in eq (22)).

For the next step in evaluating the predominant S-parameter terms in P_{net} , the system is in the configuration shown in figure 3b where the port 4 short has been replaced with the port 2 power meter, and port 2 is terminated with a matched load, ($\Gamma_2 \cong 0.05$). The ratio of the two power measurements is (analogous to eq (19))

$$\frac{P_1}{P_4} = \left| \frac{b_1}{b_4} \right|^2 \frac{1 - |\Gamma_1|^2}{1 - |\Gamma_4|^2} \quad (23)$$

where we solve eq (15) (or take the reciprocal of eq (17)) to obtain

$$\left| \frac{b_1}{b_4} \right|^2 = \left| \frac{S_{13}}{S_{34}} \right|^2 \times \left| \frac{1 - S_{44} \Gamma_4}{1 - S_{11} \Gamma_1} \right|^2 \times \left| \frac{1 + \frac{S_{14} S_{34} \Gamma_4}{S_{13} (1 - S_{44} \Gamma_4)}}{1 + \frac{S_{13} S_{14} \Gamma_1}{S_{34} (1 - S_{11} \Gamma_1)}} \right|^2 \quad (24)$$

$$\times \left| \frac{1 - \frac{(S_{13} S_{24} - S_{12} S_{34})(S_{13} S_{24} - S_{14} S_{23}) \Gamma_2 \Gamma_4}{[S_{13} (1 - S_{22} \Gamma_2) + S_{12} S_{23} \Gamma_2][S_{13} (1 - S_{44} \Gamma_4) + S_{14} S_{34} \Gamma_4]}}{1 + \frac{(S_{13} S_{24} - S_{12} S_{34})[S_{23} (1 - S_{11} \Gamma_1) + S_{12} S_{13} \Gamma_1] \Gamma_2}{[S_{13} (1 - S_{22} \Gamma_2) + S_{12} S_{23} \Gamma_2][S_{34} (1 - S_{11} \Gamma_1) + S_{13} S_{14} \Gamma_1]}} \right|^2$$

in which every Γ_2 is then set equal to 0.05. Again, because many of the S_{ij} magnitudes are small, and the phases not known, we reduce eq (24) to the form

$$\left| \frac{b_1}{b_4} \right|^2 = \left| \frac{S_{13}}{S_{34}} \right|^2 (1 \pm \Delta) \quad (25)$$

where Δ includes all that we do not know about the S_{ij} . From eqs (23,25) we now have

$$\left| \frac{S_{13}}{S_{34}} \right|^2 = \frac{P_1}{P_4 (1 \pm \Delta)} \frac{1 - |\Gamma_4|^2}{1 - |\Gamma_1|^2} \quad (26)$$

which is the predominant S-parameter dependence in $g(S, \Gamma)$ and, therefore, one of the S-parameter multipliers we need for computing P_{net} from eq (13). Again, Δ and the uncertainty in the ratio P_1/P_4 give the uncertainty in $|S_{13}/S_{34}|^2$. From eqs (22) and (26) we can now obtain a value for $|1/S_{24}|^2$ which is the predominant S-parameter dependence in $h(S, \Gamma)$.

5. Summary of Self-Calibration Procedure

In this section we summarize the computation of system S-parameters from readings of forward and reflected power at the side arms of a dual directional coupler. System self-calibration proceeds as follows.

1. We must know which parameter groups are to be evaluated. For an ideal system, eq (8) shows the S-parameters that must be known to compute

the net power to the load antenna in figure 2. For a nonideal system, eqs (13), (17), and (18) show how all the S-parameters of the system are involved in the net power measurement, and also that the S-parameters with major influence in this measurement are the same as those identified in eq (8).

2. Values for the S-parameter multipliers in eq (8) are obtained from measurements of forward and reflected power with the system in the two configurations shown in figure 3. For the system as in figure 3a, values for power measurements P_1 and P_2 and their uncertainties are entered into eq (22) to compute the quantity $|S_{24}S_{34}/S_{13}|^2$. The uncertainty Δ is computed from the last four terms in eq (20). Then, for the system as in figure 3b, power measurements P_1 and P_4 and their uncertainties are entered into eq (26) to compute the quantity $|S_{13}/S_{34}|^2$, for which the uncertainty Δ is computed from the last three terms in eq (24). We can now compute $|1/S_{24}|^2$ and its uncertainty, and thus obtain values for the leading terms in $|g|^2$ and $|h|^2$ of eq (13), where g and h are given by eqs (17) and (18).

3. The computed values for $|S_{34}/S_{13}|^2$ and $|1/S_{24}|^2$ are substituted into $|g|^2$ and $|h|^2$, respectively, in eq (13) for the net power to the load antenna in figure 2. The remaining terms in $|g|^2$ and $|h|^2$ cannot be completely evaluated because the phases of the S-parameters and reflection coefficients are not known. Therefore, each S and Γ is treated as a scalar quantity having the range of values $\pm|S|$ and $\pm|\Gamma|$, and the terms multiplying $|S_{34}/S_{13}|^2$ and $|1/S_{24}|^2$ in $|g|^2$ and $|h|^2$ are reduced to the form $1 \pm \Delta$ in the same manner as in eqs (20,21) and (24,25).

4. The total uncertainty in the net power delivered to the port 4 load has three parts which are entered into eq (13): 1) the uncertainty in the S-parameter groups $|S_{34}/S_{13}|^2$ and $|1/S_{24}|^2$ in $|g|^2$ and $|h|^2$, respectively; 2) the uncertainty, $1 \pm \Delta$, which represents our lack of knowledge of the S-parameters and reflection coefficients in the remaining terms in $|g|^2$ and $|h|^2$; and 3) the uncertainty in the power readings P_1 and P_2 .

6. Estimated Uncertainty in Computed Net Power

The uncertainty terms that we have represented by the symbol Δ are computed using nominal values for the magnitudes of S-parameters and reflection coefficients. These values are obtained from the manufacturer's specifications for the dual directional coupler and for the power sensors. Conservative values for percent uncertainty in the power meter readings are also obtained from specifications for the meter and power sensors. We have computed the estimated uncertainties using these magnitudes

$$\bullet |S_{11}| = |S_{22}| = |S_{44}| = 0.05$$

$$\bullet |S_{13}| = |S_{24}| = 0.1$$

$$\bullet |S_{14}| = |S_{23}| = 10^{-3}$$

$$\bullet |S_{12}| = 10^{-6}$$

$$\bullet |S_{34}| = 0.95$$

$$\bullet |\Gamma_1| = |\Gamma_2| = 0.05$$

$$\bullet |\Gamma_4| = 0.05 \text{ for a standard gain horn antenna (see page 14)}$$

The power meter reading contains ± 1 percent instrumentation uncertainty arising in the metering circuits, ± 1.5 percent mismatch uncertainty in the sensor calibration factor, and ± 2 percent uncertainty in the power linearity of the sensor. We therefore set a ± 4.5 percent uncertainty on each power meter reading. Using eq (13) for net power delivered to a load antenna on port 4, the system self-calibration procedure described in this report then gives an estimated worst-case uncertainty of ± 16 percent (+ 0.64 dB, - 0.75 dB) in the computed value of the delivered power P_{net} .

The quoted uncertainties in the power readings P_1 and P_2 are for a dual channel power meter with two sensors. It is possible to reduce this uncertainty by using the meter in the single channel mode (or using a single channel meter) with a single power sensor. The instrumentation uncertainty in the metering circuits is then quoted as ± 0.5 percent (instead of ± 1.0 percent). In addition, the power sensor mismatch uncertainty (a function of frequency) will cancel in the ratios P_1/P_2 and P_1/P_4 because both readings in each ratio are at the same frequency. However, the mismatch uncertainty remains in the power readings P_1 and P_2 in eq (13). A single channel power meter with one sensor reduces the estimated worst-case uncertainty in P_{net} to ± 11.4 percent (+ 0.47 dB, -0.53 dB), but at the expense of increased system complexity in

added circuits to switch the single power sensor between coupler ports 1, 2, and 4.

Although the preceding computations give an estimate of the maximum uncertainty inherent in the self-calibration method, we emphasize that the S-parameter magnitudes on page 11 describe only the dual directional coupler for which they are given. In practice, the procedures set forth in this report measure parameters for the entire system within the dashed rectangle in figure 2. For example, the S-parameter S_{24} will be the transmission coefficient not just for the path between ports 2 and 4 of the coupler, but for the path between a measurement plane on the rectangle outside port 2 and a measurement plane on the rectangle outside port 4. Physically, these measurement planes are at the power sensor for meter P_2 and at the input connector on the antenna terminating port 4.

We have also used the S and Γ magnitudes on page 11 to determine the uncertainty component which appears in P_{net} as a consequence of considering the system to be nonideal; that is, the uncertainty incurred in P_{net} through using eq (13) instead of eq (8) (the uncertainties in $P_1, P_2, |S_{34}/S_{13}|^2$, and $|1/S_{24}|^2$ being the same in each equation). To compare uncertainties in the computed P_{net} for ideal and nonideal systems, the expressions $|g|^2$ and $|h|^2$ are inserted into eq (13) in the forms

$$|g|^2 = \left| \frac{S_{34}}{S_{13}} \right|^2 (1 \pm \Delta g); \quad |h|^2 = \left| \frac{1}{S_{24}} \right|^2 (1 \pm \Delta h) \quad (27)$$

where the $|1/\Gamma_4|^2$ in $|h|^2$ is omitted because it cancels the $|\Gamma_4|^2$ in eq (13). For a nonideal system, P_{net} is then

$$P_{net} = \left| \frac{S_{34}}{S_{13}} \right|^2 \frac{P_1}{1 - |\Gamma_1|^2} (1 \pm \Delta g) - \left| \frac{1}{S_{24}} \right|^2 \frac{P_2}{1 - |\Gamma_2|^2} (1 \pm \Delta h). \quad (28)$$

Equation (8) for an ideal system is

$$P_{net} = \left| \frac{S_{34}}{S_{13}} \right|^2 \frac{P_1}{1 - |\Gamma_1|^2} - \left| \frac{1}{S_{24}} \right|^2 \frac{P_2}{1 - |\Gamma_2|^2}. \quad (8)$$

Equations (28) and (8) now closely resemble one another except for the terms $(1 \pm \Delta g)$ and $(1 \pm \Delta h)$ in eq (28). Therefore, neglecting the quantities Δg and Δh is tantamount to assuming an ideal system and identifies Δg and Δh as uncertainties in P_{net} which are overlooked in this assumption.

To obtain the uncertainty in P_{net} in eq (28) due to the uncertainty Δg in the forward power term and the uncertainty Δh in the reflected power term, we write P_1 and P_2 in terms of P_0 defined as the incident minus reflected power at port 3. Referring to figure 2, an approximation to the power $P_1/(1 - |\Gamma_1|^2)$ emerging from port 1 in a nonideal system is

$$\frac{P_1}{1 - |\Gamma_1|^2} \sim P_0 |S_{13}|^2 + P_0 |S_{34}|^2 |\Gamma_4|^2 |S_{14}|^2 \quad (29)$$

Even for $|\Gamma_4|^2 = 1$, the second term is $\sim 10^4$ times smaller than the first term, so we let

$$\frac{P_1}{1 - |\Gamma_1|^2} = P_0 |S_{13}|^2 \quad (30)$$

The approximate power emerging from port 2 in a nonideal system is

$$\frac{P_2}{1 - |\Gamma_2|^2} \sim P_0 |S_{34}|^2 |\Gamma_4|^2 |S_{24}|^2 + P_0 |S_{23}|^2 \quad (31)$$

where, for $|\Gamma_4|^2 \cong 0.05$, the second term is about 25 times smaller than the first term. Because the expression in eq (30) is then about 400 times larger than that in eq (31), we let

$$\frac{P_2}{1 - |\Gamma_2|^2} = P_0 |S_{34}|^2 |\Gamma_4|^2 |S_{24}|^2 \quad (32)$$

with negligible effect on the computed uncertainty in P_{net} .

Equations (30) and (32) are good approximations for a nonideal system, and are exact for an ideal system. Substituting eqs (30) and (32) into eq (28), we have for a nonideal system

$$\begin{aligned} P_{\text{net}} &= |S_{34}|^2 P_0 (1 \pm \Delta g) - |S_{34}|^2 |\Gamma_4|^2 P_0 (1 \pm \Delta h) \\ &= |S_{34}|^2 P_0 [(1 \pm \Delta g) - |\Gamma_4|^2 (1 \pm \Delta h)] \\ &= |S_{34}|^2 P_0 [(1 - |\Gamma_4|^2) \pm (\Delta g + |\Gamma_4|^2 \Delta h)] \end{aligned} \quad (33)$$

where the absolute uncertainties Δg and Δh are grouped to form

$$\Delta P_{\text{net}} = \pm |S_{34}|^2 P_0 (\Delta g + |\Gamma_4|^2 \Delta h) \quad (34)$$

which is the contribution to the total P_{net} uncertainty neglected in the "ideal system" assumption. As a percent of P_{net} , ΔP_{net} becomes

$$\Delta P_{\text{net}}(\%) = \pm \frac{\Delta g + |\Gamma_4|^2 \Delta h}{1 - |\Gamma_4|^2} \times 100. \quad (35)$$

Now putting eqs (30) and (32) into eq (8), we have for an ideal system

$$P_{\text{net}} = |S_{34}|^2 P_0 - |S_{34}|^2 |\Gamma_4|^2 P_0 = |S_{34}|^2 P_0 (1 - |\Gamma_4|^2). \quad (36)$$

Comparing eq (36) with the first term of eq (33) shows that the mathematical descriptions of ideal and nonideal systems give the same expression for P_{net} . However, eq (33) also gives an additional uncertainty (beyond that common to P_{net} in eqs (8) and (13)) involving the terms Δg and Δh which characterize the nonideal nature of the power delivery system.

Because Δg , Δh , and the relative size of P_1 and P_2 depend on Γ_4 , we computed $\Delta P_{\text{net}}(\%)$ for three values of $|\Gamma_4|$. Numerical values for Δg and Δh were obtained by substituting the S and Γ magnitudes into eqs (17) and (18) and consolidating the second, third, and fourth terms in each of these equations into one term of the form $(1 \pm \Delta)$. For the following values for $|\Gamma_4|$, eq (35) yields

$$\begin{aligned} \bullet \quad |\Gamma_4| &= 0.05 \quad (|\Gamma_4|^2 = 0.0025), & \Delta P_{\text{net}} &= \pm 1.2\% \\ \bullet \quad |\Gamma_4| &= 0.1 \quad (|\Gamma_4|^2 = 0.01), & \Delta P_{\text{net}} &= \pm 2.1\% \\ \bullet \quad |\Gamma_4| &= 0.224 \quad (|\Gamma_4|^2 = 0.05), & \Delta P_{\text{net}} &= \pm 5.7\% \end{aligned} \quad (37)$$

(The maximum VSWR obtained by Slayton [3] for a pyramidal horn was 1.25, for which $|\Gamma| = 0.11$. Our own measurements of $|\Gamma|^2$ for a horn and an open-ended waveguide were about 0.001 ($|\Gamma| \cong 0.03$) and 0.01 ($|\Gamma| \cong 0.1$), respectively. These values suggested those we chose for $|\Gamma_4|$.)

Referring to eq (28), the total uncertainty in P_{net} comprises ΔP_{net} and the uncertainties in the S-parameter multipliers and in P_1 and P_2 . For

smaller values of Γ_4 , ΔP_{net} is a smaller part of this uncertainty. In a power delivery system using a dual channel power meter and having $|\Gamma_4| = 0.05$, $\Delta P_{\text{net}} = \pm 1.2\%$ out of a total P_{net} uncertainty of $\pm 16\%$. If $|\Gamma_4| = 0.224$, then $\Delta P_{\text{net}} = \pm 5.7\%$ out of a total uncertainty of $\pm 23\%$. Thus when Γ_4 is small, the assumption of an ideal system (i.e., the use of eq (8) instead of eq (13) to determine P_{net}) incurs only a small discrepancy in the estimated uncertainty in P_{net} .

We are currently testing the system self-calibration procedure by computing P_{net} with eq (13) and comparing that value with a direct power measurement at port 4. Results of this work will be given in a later report.

7. Conclusion

We derived an equation for computing the net power to a load antenna using a power delivery system for which all of the S-parameters are assumed to be nonzero. An S-parameter description of the system yields equations by which the system can be self-calibrated using known terminations on port 4. When the system uses a dual channel power meter and is calibrated by the procedure described, the maximum uncertainty in P_{net} obtained from eq (28) is $\pm 16\%$ (for $|\Gamma_4| = 0.05$). This uncertainty can be reduced to 11.4 percent by using a single channel power meter. We have shown that a P_{net} computation based on the "ideal system" assumption may be sufficient if the reflection coefficient of the load on port 4 is small.

8. Acknowledgment

It is our pleasure to acknowledge the cheerful and expert assistance of Wilbur Anson who wrote and ran a computer program which allowed us to observe the behavior of $g(S, \Gamma)$ and $h(S, \Gamma)$ versus many combinations of the S_{ij} and Γ_i .

9. References

- [1] Kerns, D. M.; Beatty, R.W. Basic theory of waveguide junctions and introductory microwave network analysis. New York: Pergamon Press; 1967. 150 p.
- [2] Beatty, R. W.; Macpherson, A.C. Mismatch errors in microwave power measurements. Proc. I.R.E. 41(9): 1112-1119; 1953 September.
- [3] Slayton, W. T. Design and calibration of microwave antenna gain standards. U.S. Naval Research Laboratory, Washington, D.C. Report 4433; 1954 November. 37 p.

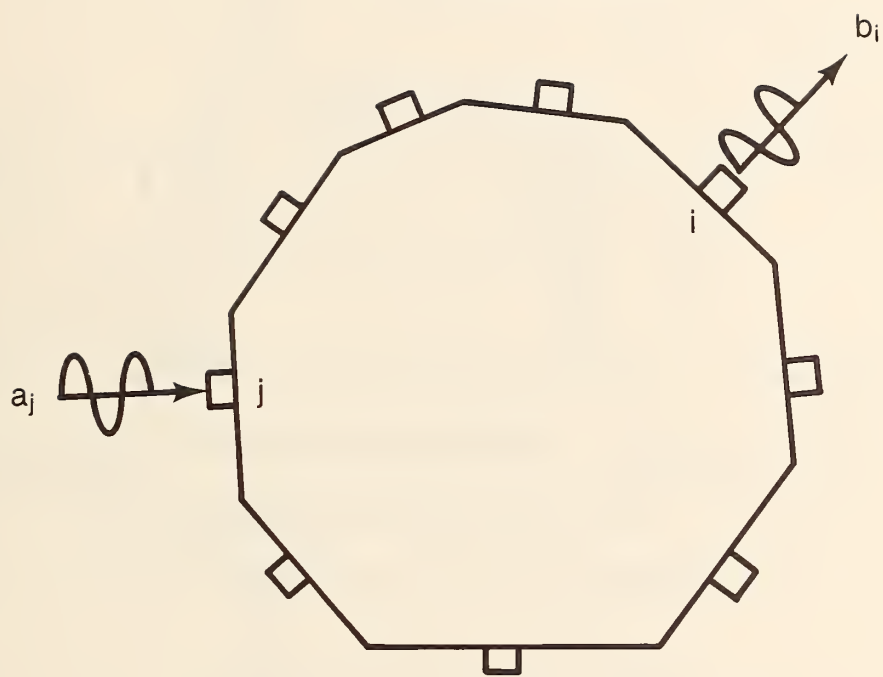


Figure 1. An n-port microwave junction

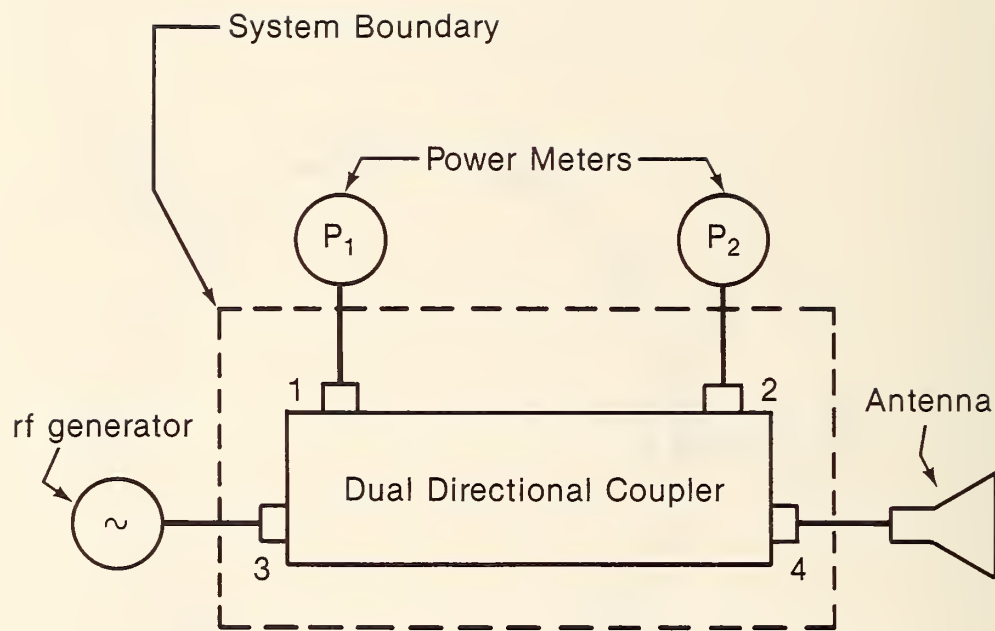


Figure 2. System for measuring rf power delivered to an antenna



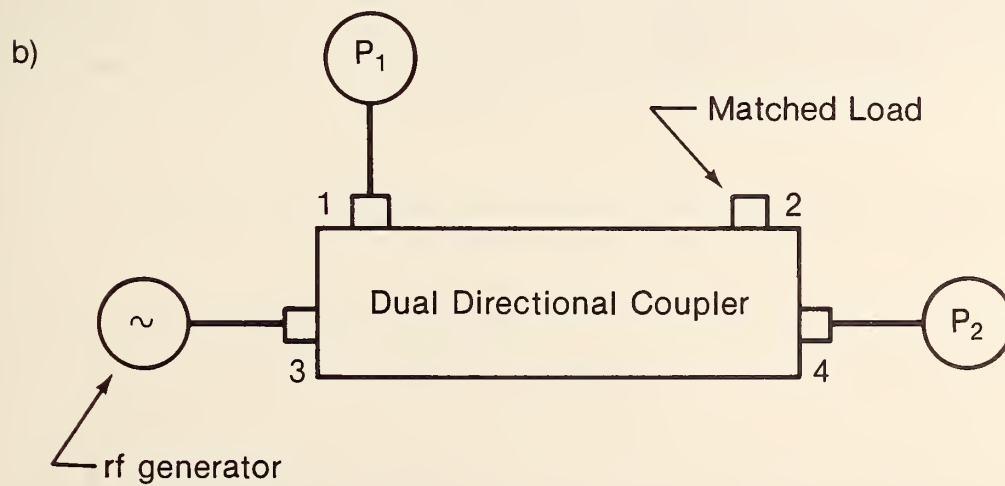


Figure 3. Configurations for measuring system s-parameters.

U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET <i>(See instructions)</i>	1. PUBLICATION OR REPORT NO. NBS TN-1083	2. Performing Organ. Report No.	3. Publication Date August 1985
4. TITLE AND SUBTITLE A Radio-Frequency Power Delivery System: Procedures for Error Analysis and Self-Calibration			
5. AUTHOR(S) Motohisa Kanda and R. David Orr			
6. PERFORMING ORGANIZATION <i>(If joint or other than NBS, see instructions)</i> NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, D.C. 20234		7. Contract/Grant No. 8. Type of Report & Period Covered	
9. SPONSORING ORGANIZATION NAME AND COMPLETE ADDRESS <i>(Street, City, State, ZIP)</i>			
10. SUPPLEMENTARY NOTES <input type="checkbox"/> Document describes a computer program; SF-185, FIPS Software Summary, is attached.			
11. ABSTRACT <i>(A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here)</i> <p>An expression is developed for net power delivered to a load in terms of the indicated forward and reflected power and the system S-parameters and reflection coefficients. The dual directional coupler is treated as nonideal with power reflections assumed between all ports. The system itself is used to evaluate the major S-parameter terms in net power computation, and uncertainty in the computed power is derived from origins in the power meter readings and incompletely known S-parameters.</p>			
12. KEY WORDS <i>(Six to twelve entries; alphabetical order; capitalize only proper names; and separate key words by semicolons)</i> errors; error analysis; radio-frequency power; scattering coefficients, S-parameters			
13. AVAILABILITY <input checked="" type="checkbox"/> Unlimited <input type="checkbox"/> For Official Distribution. Do Not Release to NTIS <input checked="" type="checkbox"/> Order From Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402. <input type="checkbox"/> Order From National Technical Information Service (NTIS), Springfield, VA. 22161			14. NO. OF PRINTED PAGES 24 15. Price

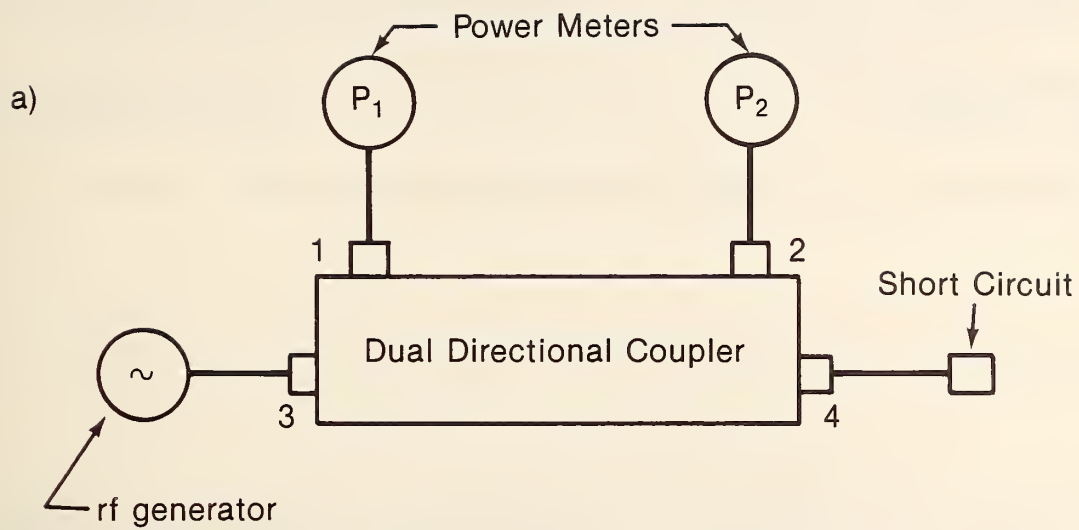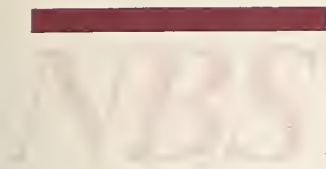

Technical Publications

Periodicals

Journal of Research—The Journal of Research of the National Bureau of Standards reports NBS research and development in those disciplines of the physical and engineering sciences in which the Bureau is active. These include physics, chemistry, engineering, mathematics, and computer sciences. Papers cover a broad range of subjects, with major emphasis on measurement methodology and the basic technology underlying standardization. Also included from time to time are survey articles on topics closely related to the Bureau's technical and scientific programs. As a special service to subscribers each issue contains complete citations to all recent Bureau publications in both NBS and non-NBS media. Issued six times a year.

Nonperiodicals

Monographs—Major contributions to the technical literature on various subjects related to the Bureau's scientific and technical activities.

Handbooks—Recommended codes of engineering and industrial practice (including safety codes) developed in cooperation with interested industries, professional organizations, and regulatory bodies.

Special Publications—Include proceedings of conferences sponsored by NBS, NBS annual reports, and other special publications appropriate to this grouping such as wall charts, pocket cards, and bibliographies.

Applied Mathematics Series—Mathematical tables, manuals, and studies of special interest to physicists, engineers, chemists, biologists, mathematicians, computer programmers, and others engaged in scientific and technical work.

National Standard Reference Data Series—Provides quantitative data on the physical and chemical properties of materials, compiled from the world's literature and critically evaluated. Developed under a worldwide program coordinated by NBS under the authority of the National Standard Data Act (Public Law 90-396).

NOTE: The Journal of Physical and Chemical Reference Data (JPCRD) is published quarterly for NBS by the American Chemical Society (ACS) and the American Institute of Physics (AIP). Subscriptions, reprints, and supplements are available from ACS, 1155 Sixteenth St., NW, Washington, DC 20056.

Building Science Series—Disseminates technical information developed at the Bureau on building materials, components, systems, and whole structures. The series presents research results, test methods, and performance criteria related to the structural and environmental functions and the durability and safety characteristics of building elements and systems.

Technical Notes—Studies or reports which are complete in themselves but restrictive in their treatment of a subject. Analogous to monographs but not so comprehensive in scope or definitive in treatment of the subject area. Often serve as a vehicle for final reports of work performed at NBS under the sponsorship of other government agencies.

Voluntary Product Standards—Developed under procedures published by the Department of Commerce in Part 10, Title 15, of the Code of Federal Regulations. The standards establish nationally recognized requirements for products, and provide all concerned interests with a basis for common understanding of the characteristics of the products. NBS administers this program as a supplement to the activities of the private sector standardizing organizations.

Consumer Information Series—Practical information, based on NBS research and experience, covering areas of interest to the consumer. Easily understandable language and illustrations provide useful background knowledge for shopping in today's technological marketplace.

Order the above NBS publications from: Superintendent of Documents, Government Printing Office, Washington, DC 20402.

Order the following NBS publications—FIPS and NBSIR's—from the National Technical Information Service, Springfield, VA 22161.

Federal Information Processing Standards Publications (FIPS PUB)—Publications in this series collectively constitute the Federal Information Processing Standards Register. The Register serves as the official source of information in the Federal Government regarding standards issued by NBS pursuant to the Federal Property and Administrative Services Act of 1949 as amended, Public Law 89-306 (79 Stat. 1127), and as implemented by Executive Order 11717 (38 FR 12315, dated May 11, 1973) and Part 6 of Title 15 CFR (Code of Federal Regulations).

NBS Interagency Reports (NBSIR)—A special series of interim or final reports on work performed by NBS for outside sponsors (both government and non-government). In general, initial distribution is handled by the sponsor; public distribution is by the National Technical Information Service, Springfield, VA 22161, in paper copy or microfiche form.

U.S. Department of Commerce
National Bureau of Standards
Gaithersburg, MD 20899

Official Business
Penalty for Private Use \$300



POSTAGE AND FEES PAID
U S DEPARTMENT OF COMMERCE
COM-215
FIRST CLASS